

Air Quality Monitoring Equipment

Date: January 23th, 2023

CALIBRATION CERTIFICATE

Equipment Name : Digital Dust Indicator, Model LD-5R
Code No. : 080000-73
Quantity : 1 unit
Serial No. : 2Y6548
Sensitivity : 0.001 mg/m³
Sensitivity Adjustment : 545 CPM
Scale Setting : November 15th, 2022.

We hereby certify that the above mentioned instrument has been calibrated satisfactory.

Sincerely

(Signature)

Tong Zhang

Tong Zhang
Overseas & New Business Group
Overseas Sales Department



Sibata LD-5R K-Factor Verification Test by Total Suspended Particulates HVS Test Report

Information of Calibrated Equipment

| | | | | | |
|-----------------------------|-----------------|----|-----------------|------------------------------|-----------------|
| Verification Test Date: | 8-Apr-23 | to | 9-Apr-23 | Next Verification Test Date: | 8-Apr-24 |
| Unit-under-Test- Model No.: | Sibata LD-5R | | | | |
| Unit-under-Test Serial No.: | 2Y6548 | | | | |
| Our Report Reference No.: | RPT-23-HVS-0045 | | | | |
| Calibration Location: | Emax | | | | |

Standard Equipment Information


| | | |
|-------------------------------|---------------|----------------------|
| Verification Equipment Type: | Tisch TSP HVS | Tisch HVS Calibrator |
| Standard Equipment Model No.: | TE-5170X | TE-5028A |
| Equipment serial no.: | 1049 | 3702 |
| Last Calibration Date: | 8-Apr-23 | 31-Mar-23 |
| Next Calibration Date: | 7-Jun-23 | 30-Mar-24 |

Equipment Verification Result

| Verification Test No. | Date | Duration | | | Results from Calibrated Equipment | | Results from Standard Equipment |
|-----------------------|----------|------------|----------|-----------------------|-----------------------------------|-----------------------|--|
| | | Start-time | End-time | Elapsed Time (in min) | Total Counts | Counts/ Minute x-axis | Dust Concentration ($\mu\text{g}/\text{m}^3$) y-axis |
| 1 | 8/4/2023 | 7339.85 | 7342.85 | 180.00 | 2520 | 14 | 44 |
| 2 | 8/4/2023 | 7342.85 | 7345.85 | 180.00 | 2040 | 11 | 36 |
| 3 | 8/4/2023 | 7345.85 | 7348.85 | 180.00 | 6240 | 35 | 97 |
| 4 | 9/4/2023 | 7349.74 | 7352.74 | 180.00 | 1440 | 8 | 29 |
| 5 | 9/4/2023 | 7352.76 | 7355.76 | 180.00 | 1740 | 10 | 31 |
| 6 | 9/4/2023 | 7355.77 | 7358.77 | 180.00 | 6000 | 33 | 102 |

Linear Regression of y on x

| | | | | | |
|---|---------------|------------|---|-----------------------------|---------------|
| Slope, K factor: | 2.7466 | Intercept: | 5.4440 | *Correlation Coefficient,R: | 0.9964 |
| Verification Test Result: <u>Strong Correlation, Results were accepted.</u> | | | * If the Correlation Coefficient, R is <0.5. Checking and Re-verification are required. | | |

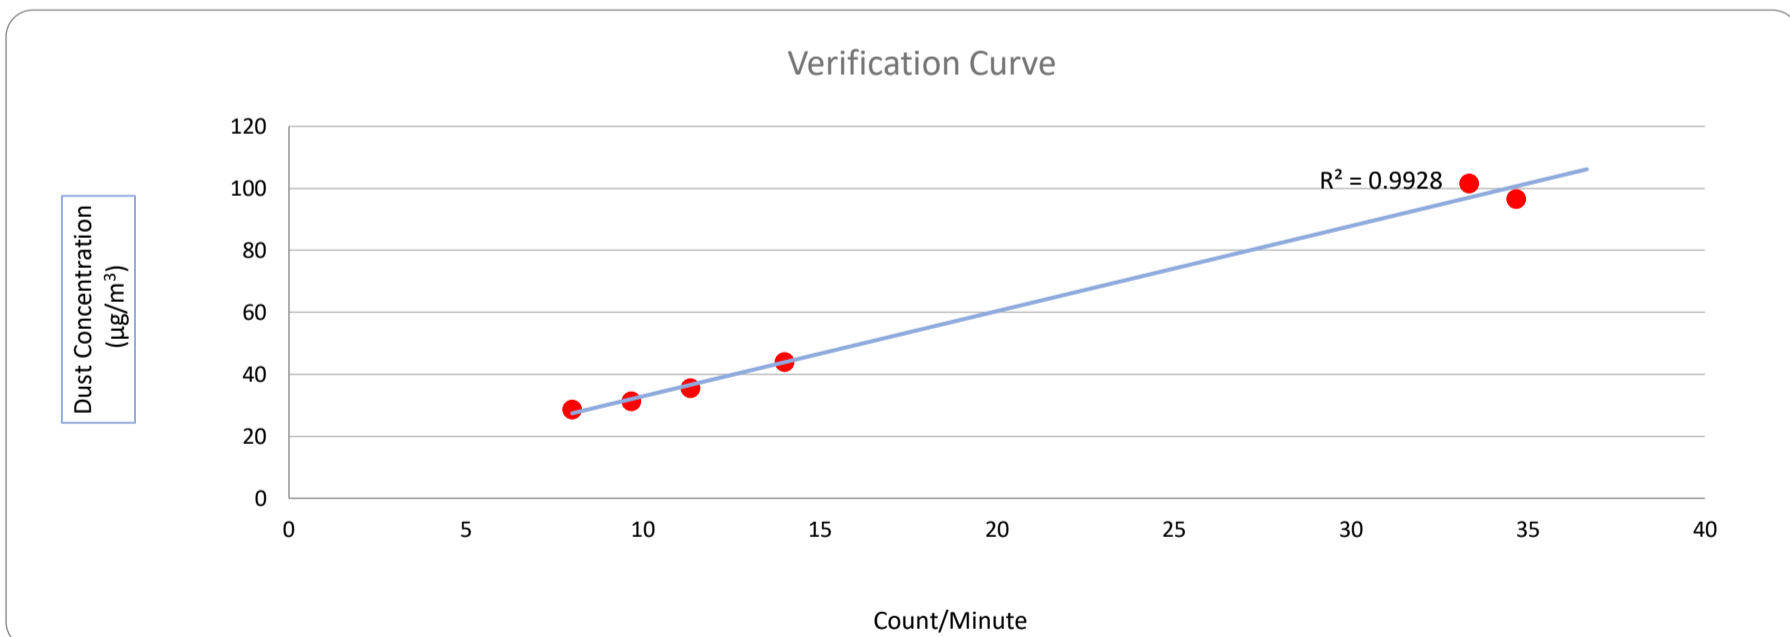

Operated By: Andy Li
Project Technician, Environmental

Date: 10-04-2023

Checked By: Tandy Tse
Senior Consultant, Environmental

Date: 10-04-2023

Date: January 23th, 2023

CALIBRATION CERTIFICATE

Equipment Name : Digital Dust Indicator, Model LD-5R
Code No. : 080000-73
Quantity : 1 unit
Serial No. : 2Y6549
Sensitivity : 0.001 mg/m³
Sensitivity Adjustment : 549 CPM
Scale Setting : November 15th, 2022.

We hereby certify that the above mentioned instrument has been calibrated satisfactory.

Sincerely

(Signature)

Tong Zhang

Tong Zhang
Overseas & New Business Group
Overseas Sales Department



Sibata LD-5R K-Factor Verification Test by Total Suspended Particulates HVS Test Report

Information of Calibrated Equipment

| | | | | | |
|-----------------------------|-----------------|----|-----------------|------------------------------|-----------------|
| Verification Test Date: | 8-Apr-23 | to | 9-Apr-23 | Next Verification Test Date: | 8-Apr-24 |
| Unit-under-Test- Model No.: | Sibata LD-5R | | | | |
| Unit-under-Test Serial No.: | 2Y6549 | | | | |
| Our Report Reference No.: | RPT-23-HVS-0046 | | | | |
| Calibration Location: | Emax | | | | |

Standard Equipment Information


| | | |
|-------------------------------|---------------|----------------------|
| Verification Equipment Type: | Tisch TSP HVS | Tisch HVS Calibrator |
| Standard Equipment Model No.: | TE-5170X | TE-5028A |
| Equipment serial no.: | 1049 | 3702 |
| Last Calibration Date: | 8-Apr-23 | 31-Mar-23 |
| Next Calibration Date: | 7-Jun-23 | 30-Mar-24 |

Equipment Verification Result

| Verification Test No. | Date | Duration | | | Results from Calibrated Equipment | | Results from Standard Equipment |
|-----------------------|----------|------------|----------|-----------------------|-----------------------------------|-----------------------|--|
| | | Start-time | End-time | Elapsed Time (in min) | Total Counts | Counts/ Minute x-axis | Dust Concentration ($\mu\text{g}/\text{m}^3$) y-axis |
| 1 | 8/4/2023 | 7339.85 | 7342.85 | 180.00 | 2760 | 15 | 44 |
| 2 | 8/4/2023 | 7342.85 | 7345.85 | 180.00 | 2220 | 12 | 36 |
| 3 | 8/4/2023 | 7345.85 | 7348.85 | 180.00 | 5940 | 33 | 97 |
| 4 | 9/4/2023 | 7349.74 | 7352.74 | 180.00 | 1740 | 10 | 29 |
| 5 | 9/4/2023 | 7352.76 | 7355.76 | 180.00 | 1980 | 11 | 31 |
| 6 | 9/4/2023 | 7355.77 | 7358.77 | 180.00 | 5760 | 32 | 102 |

Linear Regression of y on x

| | | | | | |
|---|---------------|------------|----------------|---|---------------|
| Slope, K factor: | 3.1227 | Intercept: | -2.7291 | *Correlation Coefficient,R: | 0.9968 |
| Verification Test Result: <u>Strong Correlation, Results were accepted.</u> | | | | * If the Correlation Coefficient, R is <0.5. Checking and Re-verification are required. | |

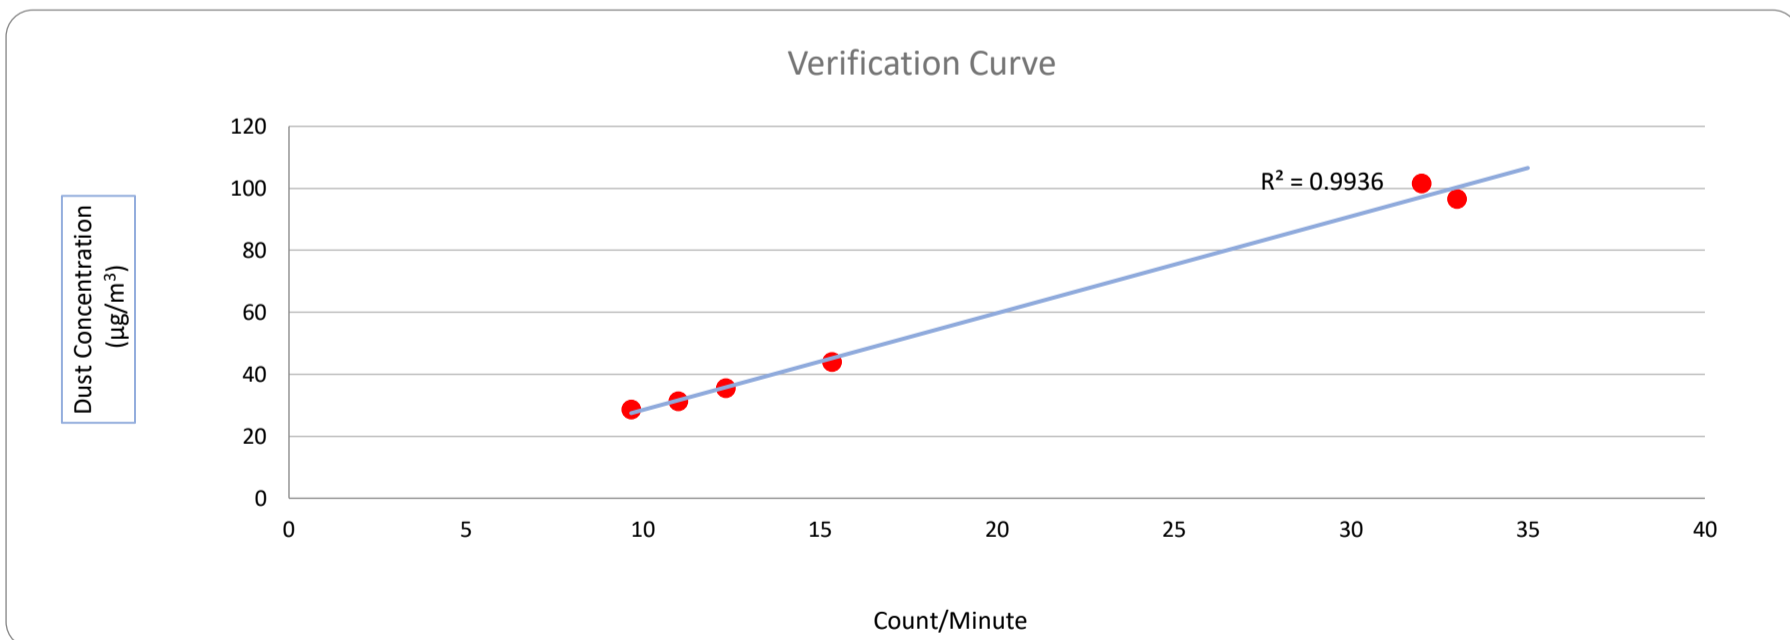

Operated By: Andy Li
Project Technician, Environmental

Date: 10-04-2023

Checked By: Tandy Tse
Senior Consultant, Environmental

Date: 10-04-2023

Noise Quality Monitoring Equipment



Certificate of Calibration

for

Description: *Sound Level Calibrator*
Manufacturer: *RION*
Type No.: *NC-74*
Serial No.: *34615222*

Submitted by:

Customer: *Acuity Sustainability Consulting Limited*
Address: *Unit E, 12/F, Ford Glory Plaza,
Nos. 37-39 Wing Hong Street,
Cheung Sha Wan, Kowloon,
Hong Kong*

Upon receipt for calibration, the instrument was found to be:

- Within**
 Outside

the allowable tolerance.

The test equipments used for calibration are traceable to National Standards via:


- The Government of The Hong Kong Special Administrative Region Standard & Calibration Laboratory

Date of receipt: 16 March 2023

Date of calibration: 21 March 2023

Date of NEXT calibration: 20 March 2024

Calibrated by: 
Calibration Technician

Certified by: 
*Mr. Ng Yan Wa
Laboratory Manager*

Date of issue: 21 March 2023

Certificate No.: APJ22-157-CC004



1. Calibration Precautions:

- The unit-under-test (UUT) was allowed to stabilize in the laboratory for over 24 hours, and switched on to warm up for over 10 minutes before the commencement of the test.
- The results presented are the mean of 3 measurements at each calibration point.

2. Calibration Specifications:

Calibration check

3. Calibration Conditions:

Air Temperature: 22.1 °C
Air Pressure: 1006 hPa
Relative Humidity: 61.7 %

4. Calibration Equipment:

| Test Equipment | Type | Serial No. | Calibration Report Number | Traceable to |
|--------------------------|------------|------------|---------------------------|--------------|
| Multifunction Calibrator | B&K 4226 | 2288467 | AV220061 | HOKLAS |
| Sound Level Meter | RION NA-28 | 30721812 | AV220120 | HOKLAS |

5. Calibration Results

5.1 Sound Pressure Level

| Nominal value dB | Accept lower level dB | Accept upper level dB | Measured value dB |
|---------------------|--------------------------|--------------------------|----------------------|
| 94.0 | 93.6 | 94.4 | 93.9 |

Note:

The values given in this certification only related to the values measured at the time of the calibration.



Cal Lab Limited 校正實驗室有限公司

Room 2103, Technology Plaza, 29-35 Sha Tsui Road,
Tsuen Wan, NT, Hong Kong

Tel: +852 25680106 Email: info@callab.com.hk

Fax: +852 30116194 Website: www.callab.com.hk



Calibration Certificate No.: CC0292304

Customer Information

Customer: Acuity Sustainability Consulting Limited

Address: Unit E, 12/F, Ford Glory Plaza, Nos. 37-39 Wing Hong Street, Cheung Sha Wan, Kowloon, Hong Kong

Equipment Identification

| Equipment Description | Manufacturer | Model No. | Serial No. | Assigned equipment No. |
|-----------------------|--------------|-----------|------------|------------------------|
| Air Velocity Monitor | RS PRO | RS-90 | 210722153 | ASCL-EQ-110 |

Certificate Information

| | | | |
|--------------------------|---------------|------------------------|------------------------|
| Date of Receipt: | 24 April 2023 | Calibration Condition: | 23.3°C, 57%RH, 1002hPa |
| Date of Calibration: | 5 May 2023 | Adjustment: | N/A |
| Due Date of Calibration: | N/A | Appearance: | Good |
| Calibration Procedure: | SOP-112 | Remark: | N/A |

Reference Equipment Identification

| Equipment Description | Model | Serial No. | Expiration Date |
|-----------------------|-------|--------------|-----------------|
| Hot Wire Anemometer | 9535 | T95351316004 | 11 August 2024 |

Result of Calibration

Air flow rate

| Reference reading (m/s) | Measured reading (m/s) | Error (%) | Uncertainty (%FS) | Technical Requirement (m/s) | Technical Reference Doc. |
|-------------------------|------------------------|-----------|-------------------|-----------------------------|--------------------------|
| 1.02 | 1.03 | 1.0 | 3.6 | ± 0.33 | Mfr's Spec. |
| 2.99 | 2.97 | -0.7 | 3.6 | ± 0.39 | Mfr's Spec. |
| 5.03 | 4.92 | -2.2 | 3.6 | ± 0.45 | Mfr's Spec. |
| 6.98 | 6.86 | -1.7 | 3.6 | ± 0.51 | Mfr's Spec. |
| 9.97 | 9.76 | -2.1 | 3.6 | ± 0.60 | Mfr's Spec. |

CT-AFR-01

- Note1: The estimated expanded uncertainties have been calculated in "Evaluation and expression of uncertainty in measurement" and give an internal estimated to have a level of confidence of 95%. A coverage factor of 2 is assumed unless explicitly stated.
- Note2: The standard (s) and instrument used in the calibration are traceable to national or international recognized standard and are calibrated on a schedule to maintain the accuracy and good condition.
- Note3: The result reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the long term stability of the instrument.
- Note4: The result shows in this calibration certificate relate only to the item calibrated, and the result only applies to the calibration item as received.

Calibrated By:

Wing Cheng

Checked and Approved By:

Warren Yeung

Company Chop:



Certificate Issue Date: 5 May 2023

*** End of Certificate ***

CT-BEG-03

- The certificate shall not be reproduced except in full, without written approval of Cal Lab Calibration
- The certificate is issued subject to the latest Terms and Conditions, available at our web site

CC0292304

Page 1 of 1

Certificate of Calibration

for

Description: *Sound Level Calibrator*
Manufacturer: *SVANTEK*
Type No.: *SV33B*
Serial No.: *83042*

Submitted by:

Customer: *Acuity Sustainability Consulting Limited*
Address: *Unit E, 12/F, Ford Glory Plaza,
Nos. 37-39 Wing Hong Street,
Cheung Sha Wan, Kowloon,
Hong Kong*

Upon receipt for calibration, the instrument was found to be:

- Within**
 Outside

the allowable tolerance.


The test equipments used for calibration are traceable to National Standards via:


- The Government of The Hong Kong Special Administrative Region Standard & Calibration Laboratory

Date of receipt: 2 May 2023

Date of calibration: 9 May 2023

Date of NEXT calibration: 8 May 2024

Calibrated by: 
Calibration Technician

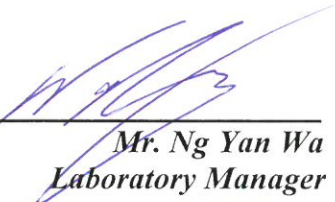Certified by: 
Mr. Ng Yan Wa
Laboratory Manager

Date of issue: 9 May 2023

Certificate No.: APJ22-157-CC005



Page 1 of 2

1. Calibration Precautions:

- The unit-under-test (UUT) was allowed to stabilize in the laboratory for over 24 hours, and switched on to warm up for over 10 minutes before the commencement of the test.
- The results presented are the mean of 3 measurements at each calibration point.

2. Calibration Specifications:

Calibration check

3. Calibration Conditions:

Air Temperature: 22.4 °C
Air Pressure: 1006 hPa
Relative Humidity: 60.9 %

4. Calibration Equipment:

| Test Equipment | Type | Serial No. | Calibration Report Number | Traceable to |
|--------------------------|------------|------------|---------------------------|--------------|
| Multifunction Calibrator | B&K 4226 | 2288467 | AV220061 | HOKLAS |
| Sound Level Meter | RION NA-28 | 30721812 | AV220120 | HOKLAS |

5. Calibration Results

5.1 Sound Pressure Level

| Nominal value dB | Accept lower level dB | Accept upper level dB | Measured value dB |
|---------------------|--------------------------|--------------------------|----------------------|
| 114.0 | 113.6 | 114.4 | 114.2 |

Note:

The values given in this certification only related to the values measured at the time of the calibration.



Certificate of Calibration

for

Description: *Sound Level Meter*
Manufacturer: *NTi Audio*
Type No.: *XL2 (Serial No.: A2A-13548-E0)*
Microphone: *ACO 7052 (Serial No.:73912)*
Preamplifier: *NTi Audio M2211 MA220 (Serial No.:5735)*

Submitted by:

Customer: *Acuity Sustainability Consulting Limited*
Address: *Unit E, 12/F, Ford Glory Plaza,
Nos. 37-39 Wing Hong Street,
Cheung Sha Wan, Kowloon, Hong Kong*

Upon receipt for calibration, the instrument was found to be:

- Within (31.5Hz – 8kHz)**
 Outside

the allowable tolerance.

The test equipment used for calibration are traceable to National Standards via:

- The Government of The Hong Kong Special Administrative Region Standard & Calibration Laboratory

Date of receipt: 2 February 2023

Date of calibration: 6 February 2023

Date of NEXT calibration: 5 February 2024

Calibrated by: _____
Calibration Technician

Certified by: _____
*Mr. Ng Yan Wa
Laboratory Manager*

Date of issue: 6 February 2023

Certificate No.: APJ22-124-CC001



Page 1 of 4

1. Calibration Precaution:

- The unit-under-test (UUT) was allowed to stabilize in the laboratory for over 24 hours, and switched on to warm up for over 10 minutes before the commencement of the test.
- The results presented are the mean of 3 measurements at each calibration point.

2. Calibration Conditions:

Air Temperature: 23.9 °C
 Air Pressure: 1006 hPa
 Relative Humidity: 47.9 %

3. Calibration Equipment:

| | Type | Serial No. | Calibration Report Number | Traceable to |
|--------------------------|----------|------------|---------------------------|--------------|
| Multifunction Calibrator | B&K 4226 | 2288467 | AV220061 | HOKLAS |

4. Calibration Results

Sound Pressure Level

Reference Sound Pressure Level

| Setting of Unit-under-test (UUT) | | | | Applied value | | UUT Reading, dB | IEC 61672 Class 1 Specification, dB |
|----------------------------------|-----------------|----------------|-----------|---------------|------|-----------------|-------------------------------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | | | |
| 30-130 | dBA SPL | Fast | 94 | 1000 | 94.1 | ±0.4 | |


Linearity

| Setting of Unit-under-test (UUT) | | | | Applied value | | UUT Reading, dB | IEC 61672 Class 1 Specification, dB |
|----------------------------------|-----------------|----------------|-----------|---------------|-------|-----------------|-------------------------------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | | | |
| 30-130 | dBA SPL | Fast | 94 | 1000 | 94.1 | Ref | |
| | | | 104 | | 104.1 | ±0.3 | |
| | | | 114 | | 114.1 | ±0.3 | |

Time Weighting

| Setting of Unit-under-test (UUT) | | | | Applied value | | UUT Reading, dB | IEC 61672 Class 1 Specification, dB |
|----------------------------------|-----------------|----------------|-----------|---------------|------|-----------------|-------------------------------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | | | |
| 30-130 | dBA SPL | Fast | 94 | 1000 | 94.1 | Ref | |
| | | Slow | | | 94.1 | ±0.3 | |

Certificate No.: APJ22-124-CC001



Page 2 of 4

Frequency Response

Linear Response

| Setting of Unit-under-test (UUT) | | | Applied value | | UUT Reading, dB | IEC 61672 Class 1 Specification, dB | |
|----------------------------------|-----------------|----------------|---------------|---------------|--------------------|--|------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | | | |
| 30-130 | dB | SPL | 94 | Fast | 31.5 | 94.1 | ±2.0 |
| | | | | | 63 | 94.2 | ±1.5 |
| | | | | | 125 | 94.1 | ±1.5 |
| | | | | | 250 | 94.1 | ±1.4 |
| | | | | | 500 | 94.2 | ±1.4 |
| | | | | | 1000 | 94.1 | Ref |
| | | | | | 2000 | 94.5 | ±1.6 |
| | | | | | 4000 | 95.2 | ±1.6 |
| | | | | | 8000 | 94.9 | +2.1; -3.1 |

A-weighting

| Setting of Unit-under-test (UUT) | | | Applied value | | UUT Reading, dB | IEC 61672 Class 1 Specification, dB | |
|----------------------------------|-----------------|----------------|---------------|---------------|--------------------|--|----------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | | | |
| 30-130 | dBA | SPL | 94 | Fast | 31.5 | 54.8 | -39.4±2.0 |
| | | | | | 63 | 68.0 | -26.2±1.5 |
| | | | | | 125 | 78.0 | -16.1±1.5 |
| | | | | | 250 | 85.5 | -8.6±1.4 |
| | | | | | 500 | 91.0 | -3.2±1.4 |
| | | | | | 1000 | 94.1 | Ref |
| | | | | | 2000 | 95.7 | +1.2±1.6 |
| | | | | | 4000 | 96.2 | +1.0±1.6 |
| | | | | | 8000 | 93.9 | -1.1±2.1; -3.1 |

C-weighting

| Setting of Unit-under-test (UUT) | | | Applied value | | UUT Reading, dB | IEC 61672 Class 1 Specification, dB | |
|----------------------------------|-----------------|----------------|---------------|---------------|--------------------|--|-----------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | | | |
| 30-130 | dBC | SPL | 94 | Fast | 31.5 | 91.2 | -3.0±2.0 |
| | | | | | 63 | 93.4 | -0.8±1.5 |
| | | | | | 125 | 94.0 | -0.2±1.5 |
| | | | | | 250 | 94.1 | -0.0±1.4 |
| | | | | | 500 | 94.2 | -0.0±1.4 |
| | | | | | 1000 | 94.1 | Ref |
| | | | | | 2000 | 94.3 | -0.2±1.6 |
| | | | | | 4000 | 94.4 | -0.8±1.6 |
| | | | | | 8000 | 92.0 | -3.0 +2.1; -3.1 |

Certificate No.: APJ22-124-CC001



Page 3 of 4

5. Calibration Results Applied

The results apply to the particular unit-under-test only. All calibration points are within manufacture's specification as IEC 61672 Class 1.

Uncertainties of Applied Value:

| | | |
|--------|---------|--------|
| 94 dB | 31.5 Hz | ± 0.10 |
| | 63 Hz | ± 0.10 |
| | 125 Hz | ± 0.10 |
| | 250 Hz | ± 0.05 |
| | 500 Hz | ± 0.10 |
| | 1000 Hz | ± 0.05 |
| | 2000 Hz | ± 0.05 |
| | 4000 Hz | ± 0.05 |
| | 8000 Hz | ± 0.10 |
| 104 dB | 1000 Hz | ± 0.05 |
| 114 dB | 1000 Hz | ± 0.05 |

The uncertainties are evaluated for a 95% confidence level.

Note:

The values given in this certification only related to the values measured at the time of the calibration and any uncertainties quoted will not allow for the equipment long-term drift, variations with environmental changes, vibration and shock during transportation, overloading, mis-handling, or the capability of any other laboratory to repeat the calibration. (A+A)*L shall not be liable for any loss or damage resulting from the use of the equipment.

Manufacturer Calibration Certificate

The following instrument has been tested and calibrated to the manufacturer specifications.
The calibration is traceable in accordance with ISO/IEC 17025 covering all instrument functions.

- Device Type: **XL2 Audio and Acoustic Analyzer**
- Serial Number: **A2A-13663-F0**

- Certificate Issued: **15 February 2023**
- Certificate Number: **44972-A2A-13663-F0**
- Results: **PASSED**
(for detailed report see next page)

Tested by:

M. Frick

Signature:

Stamp:



NTi Audio AG
Im alten Riet 102
LI - 0494 Schaan
www.nti-audio.com

Calibration of: XL2 Audio and Acoustic Analyzer
 Serial Number: A2A-13663-F0
 Date: 15 February 2023

• Detailed Calibration Test Results:

| | reference | actual | unit | actual error | XL2 tolerance | calibration uncertainty ² |
|----------------------------------|-----------|------------------|------|--------------|---------------|--------------------------------------|
| RMS Level @ 1kHz, XLR Input | 0.1 | 0.100 | V | ≤0.1% | ±0.5% | ±0.10% |
| | 1 | 0.999 | V | -0.1% | ±0.5% | ±0.09% |
| | 10 | 9.982 | V | -0.2% | ±0.5% | ±0.09% |
| Flatness, XLR Input ¹ | 20 Hz | 0.995 | V | -0.5% | ±1.1% | ±0.09% |
| | 20 kHz | 1.003 | V | 0.3% | ±1.1% | ±0.09% |
| Frequency | 1000 | 1000.00 | Hz | ≤0.003% | ±0.003% | ±0.01% |
| Residual Noise | XLR | < 2 uV | | | <2 uV | ±0.50% |
| THD+N @ 0 dBu, 1 kHz, XLR Input | | -100.5 | dB | | typ. -100 dB | ±0.50% |

- Test Conditions: Temperature: **24.9** °C
 Relative Humidity: **19.8** %

• Calibration Equipment Used:

- Agilent Multimeter, Typ 34401A, Serial No. MY 5300 4607
 Last calibration: 15.09.2022, Next calibration: 15.09.2023
 Calibrated by ELCAL to the national standards maintained at Swiss Federal Office of Metrology. SCS 0002
- FX100 Audio Analyzer, Serial No. 10408
 Last Calibration: 11.10.2022, Next Calibration: 11.10.2023
 Manufacturer calibration based on Agilent 34410, Serial No. MY47014254,
 Last Calibration: 26.05.2022, Next Calibration: 26.05.2023
 which is calibrated by ELCAL to national standards maintained at Swiss Federal Office of Metrology. SCS 002

¹ The specified tolerance +/-0.1 dB @ 1V = +/- 1.1%

² The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%. The uncertainty evaluation has been carried out in accordance with the regulations of the GUM.

Certificate of Calibration

for

Description: *Sound Level Meter*
Manufacturer: *NTi Audio*
Type No.: *XL2 (Serial No.: A2A-17638-E0)*
Microphone: *ACO 7052 (Serial No.:84413)*
Preamplifier: *NTi Audio M2211 MA220 (Serial No.:7014)*

Submitted by:

Customer: *Acuity Sustainability Consulting Limited*
Address: *Unit E, 12/F, Ford Glory Plaza,
Nos. 37-39 Wing Hong Street,
Cheung Sha Wan, Kowloon, Hong Kong*

Upon receipt for calibration, the instrument was found to be:

- Within (31.5Hz – 8kHz)**
 Outside

the allowable tolerance.

The test equipment used for calibration are traceable to National Standards via:

- The Government of The Hong Kong Special Administrative Region Standard & Calibration Laboratory

Date of receipt: 30 March 2023

Date of calibration: 04 April 2023

Date of NEXT calibration: 03 April 2024

Calibrated by: _____
Calibration Technician

Certified by: _____
*Mr. Ng Yan Wa
Laboratory Manager*

Date of issue: 04 April 2023

Certificate No.: APJ22-164-CC001



Page 1 of 4

1. Calibration Precaution:

- The unit-under-test (UUT) was allowed to stabilize in the laboratory for over 24 hours, and switched on to warm up for over 10 minutes before the commencement of the test.
- The results presented are the mean of 3 measurements at each calibration point.

2. Calibration Conditions:

Air Temperature: 21.6 °C
 Air Pressure: 1005 hPa
 Relative Humidity: 71.6 %

3. Calibration Equipment:

| | Type | Serial No. | Calibration Report Number | Traceable to |
|--------------------------|----------|------------|---------------------------|--------------|
| Multifunction Calibrator | B&K 4226 | 2288467 | AV220061 | HOKLAS |

4. Calibration Results

Sound Pressure Level

Reference Sound Pressure Level

| Setting of Unit-under-test (UUT) | | | | Applied value | | UUT Reading, dB | IEC 61672 Class 1 Specification, dB |
|----------------------------------|-----------------|----------------|-----------|---------------|------|-----------------|-------------------------------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | | | |
| 30-130 | dBA SPL | Fast | 94 | 1000 | 94.1 | ±0.4 | |


Linearity

| Setting of Unit-under-test (UUT) | | | | Applied value | | UUT Reading, dB | IEC 61672 Class 1 Specification, dB |
|----------------------------------|-----------------|----------------|-----------|---------------|-------|-----------------|-------------------------------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | | | |
| 30-130 | dBA SPL | Fast | 94 | 1000 | 94.1 | Ref | |
| | | | 104 | | 104.1 | ±0.3 | |
| | | | 114 | | 114.1 | ±0.3 | |

Time Weighting

| Setting of Unit-under-test (UUT) | | | | Applied value | | UUT Reading, dB | IEC 61672 Class 1 Specification, dB |
|----------------------------------|-----------------|----------------|-----------|---------------|------|-----------------|-------------------------------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | | | |
| 30-130 | dBA SPL | Fast | 94 | 1000 | 94.1 | Ref | |
| | | Slow | | | 94.1 | ±0.3 | |

Certificate No.: APJ22-164-CC001



Page 2 of 4

Frequency Response

Linear Response

| Setting of Unit-under-test (UUT) | | | Applied value | | UUT Reading, dB | IEC 61672 Class 1 Specification, dB | |
|----------------------------------|-----------------|----------------|---------------|---------------|--------------------|--|------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | | | |
| 30-130 | dB | SPL | Fast | 94 | 31.5 | 94.1 | ±2.0 |
| | | | | | 63 | 94.1 | ±1.5 |
| | | | | | 125 | 94.1 | ±1.5 |
| | | | | | 250 | 94.0 | ±1.4 |
| | | | | | 500 | 94.1 | ±1.4 |
| | | | | | 1000 | 94.1 | Ref |
| | | | | | 2000 | 94.3 | ±1.6 |
| | | | | | 4000 | 94.9 | ±1.6 |
| | | | | | 8000 | 93.9 | +2.1; -3.1 |

A-weighting

| Setting of Unit-under-test (UUT) | | | Applied value | | UUT Reading, dB | IEC 61672 Class 1 Specification, dB | |
|----------------------------------|-----------------|----------------|---------------|---------------|--------------------|--|----------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | | | |
| 30-130 | dBA | SPL | Fast | 94 | 31.5 | 54.7 | -39.4±2.0 |
| | | | | | 63 | 67.9 | -26.2±1.5 |
| | | | | | 125 | 78.0 | -16.1±1.5 |
| | | | | | 250 | 85.4 | -8.6±1.4 |
| | | | | | 500 | 90.9 | -3.2±1.4 |
| | | | | | 1000 | 94.1 | Ref |
| | | | | | 2000 | 95.5 | +1.2±1.6 |
| | | | | | 4000 | 95.9 | +1.0±1.6 |
| | | | | | 8000 | 92.8 | -1.1+2.1; -3.1 |

C-weighting

| Setting of Unit-under-test (UUT) | | | Applied value | | UUT Reading, dB | IEC 61672 Class 1 Specification, dB | |
|----------------------------------|-----------------|----------------|---------------|---------------|--------------------|--|-----------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | | | |
| 30-130 | dBC | SPL | Fast | 94 | 31.5 | 91.0 | -3.0±2.0 |
| | | | | | 63 | 93.3 | -0.8±1.5 |
| | | | | | 125 | 93.9 | -0.2±1.5 |
| | | | | | 250 | 94.1 | -0.0±1.4 |
| | | | | | 500 | 94.2 | -0.0±1.4 |
| | | | | | 1000 | 94.1 | Ref |
| | | | | | 2000 | 94.2 | -0.2±1.6 |
| | | | | | 4000 | 94.1 | -0.8±1.6 |
| | | | | | 8000 | 90.9 | -3.0 +2.1: -3.1 |

Certificate No.: APJ22-164-CC001



Page 3 of 4

5. Calibration Results Applied

The results apply to the particular unit-under-test only. All calibration points are within manufacture's specification as IEC 61672 Class 1.

Uncertainties of Applied Value:


| | | |
|--------|---------|--------|
| 94 dB | 31.5 Hz | ± 0.10 |
| | 63 Hz | ± 0.10 |
| | 125 Hz | ± 0.05 |
| | 250 Hz | ± 0.05 |
| | 500 Hz | ± 0.05 |
| | 1000 Hz | ± 0.05 |
| | 2000 Hz | ± 0.05 |
| | 4000 Hz | ± 0.05 |
| | 8000 Hz | ± 0.10 |
| 104 dB | 1000 Hz | ± 0.05 |
| 114 dB | 1000 Hz | ± 0.05 |

The uncertainties are evaluated for a 95% confidence level.

Note:

The values given in this certification only related to the values measured at the time of the calibration and any uncertainties quoted will not allow for the equipment long-term drift, variations with environmental changes, vibration and shock during transportation, overloading, mis-handling, or the capability of any other laboratory to repeat the calibration. (A+A)*L shall not be liable for any loss or damage resulting from the use of the equipment.

Water Quality Monitoring Equipment



專業化驗有限公司
QUALITY PRO TEST-CONSULT LIMITED

Unit 10, 5/F, Wah Wai Centre, 38-40 Au Pui Wan St., Fotan, Hong Kong
Email: info@qualityprotest.com; Website: www.qualityprotest.com
Tel: (852) 3956 8717; Fax: (852) 3956 3928

REPORT OF EQUIPMENT PERFORMANCE CHECK/ CALIBRATION

Test Report No. : R-BC120002
Date of Issue : 05 December 2023
Page No. : 1 of 2

PART A - CUSTOMER INFORMATION

Acuity Sustainability Consulting Limited
Unit E, 12/F, Ford Glory Plaza 37-39 Wing Hong Street, Cheung Sha Wan, Kowloon, Hong Kong

PART B - SAMPLE INFORMATION

Name of Equipment : YSI ProDSS (Multi-Parameters)
Manufacturer : YSI (a xylem brand)
Serial Number : 22D100436
Date of Received : 01 December 2023
Date of Calibration : 04 December 2023
Date of Next Calibration : 03 March 2024
Request No. : D-BC120002

PART C - REFERENCE METHODS/ DOCUMENTS FOR THE CALIBRATION

| Test Parameter | Reference Method |
|------------------|---|
| pH value | APHA 21e 4500-H ⁺ B |
| Temperature | Section 6 of international Accreditation New Zealand Technical Guide no. 3 Second edition March 2008: Working Thermometer Calibration Procedure |
| Salinity | APHA 21e 2520 B |
| Dissolved oxygen | APHA 23e 4500-O G (Membrane Electrode Method) |
| Turbidity | APHA 21e 2130 B (Nephelometric Method) |

PART D - CALIBRATION RESULT

(1) pH value

| Target (pH unit) | Display Reading (pH unit) | Tolerance | Result |
|------------------|---------------------------|-----------|--------------|
| 4.00 | 4.13 | 0.13 | Satisfactory |
| 7.42 | 7.45 | 0.03 | Satisfactory |
| 10.01 | 10.02 | 0.01 | Satisfactory |

Tolerance of pH value should be less than ± 0.2 (pH unit)

(2) Temperature

| Reading of Ref. thermometer (°C) | Display Reading (°C) | Tolerance | Result |
|----------------------------------|----------------------|-----------|--------------|
| 36 | 35.5 | -0.5 | Satisfactory |
| 25 | 24.8 | -0.2 | Satisfactory |
| 15 | 15.1 | 0.1 | Satisfactory |

Tolerance of Temperature should be less than ± 2.0 (°C)

(3) Salinity


| Expected Reading (g/L) | Display Reading (g/L) | Tolerance (%) | Result |
|------------------------|-----------------------|---------------|--------------|
| 10 | 9.57 | -4.30 | Satisfactory |
| 20 | 19.14 | -4.30 | Satisfactory |
| 30 | 29.99 | -0.03 | Satisfactory |

Tolerance of Salinity should be less than ± 10.0 (%)

--- CONTINUED ON NEXT PAGE ---

AUTHORIZED
SIGNATORY:


LEE Chun-ning
Assistant Manager



專業化驗有限公司
QUALITY PRO TEST-CONSULT LIMITED

Unit 10, 5/F, Wah Wai Centre, 38-40 Au Pui Wan St., Fotan, Hong Kong
Email: info@qualityprotest.com; Website: www.qualityprotest.com
Tel: (852) 3956 8717; Fax: (852) 3956 3928

REPORT OF EQUIPMENT PERFORMANCE CHECK/ CALIBRATION

Test Report No. : R-BC120002
Date of Issue : 05 December 2023
Page No. : 2 of 2

(4) Dissolved oxygen

| Expected Reading (mg/L) | Display Reading (mg/L) | Tolerance | Result |
|---------------------------|--------------------------|-----------|--------------|
| 7.99 | 8.35 | 0.36 | Satisfactory |
| 5.00 | 5.10 | 0.10 | Satisfactory |
| 2.58 | 2.40 | -0.18 | Satisfactory |
| 0.10 | 0.20 | 0.10 | Satisfactory |

Tolerance of Dissolved oxygen should be less than ± 0.5 (mg/L)

(5) Turbidity


| Expected Reading (NTU) | Display Reading (NTU) | Tolerance (%) | Result |
|--------------------------|-------------------------|-----------------|--------------|
| 0 | 0.50 | -- | Satisfactory |
| 10 | 9.88 | -1.2 | Satisfactory |
| 20 | 18.35 | -8.2 | Satisfactory |
| 100 | 95.10 | -4.9 | Satisfactory |
| 800 | 736.55 | -7.9 | Satisfactory |

Tolerance of Turbidity should be less than ± 10.0 (%)

Remark(s)

- The "Date of Next Calibration" is recommended according to best practice principals as practiced by QPT or quoted from relevant international standards.
- The results relate only to the calibrated equipment as received
- The performance of the equipment stated in this report is checked with independent reference material and results compared against a calibrated secondary source.
- "Displayed Reading" denotes the figure shown on item under calibration/ checking regardless of equipment precision or significant figures.
- The "Tolerance Limit" mentioned is the acceptance criteria applicable for similar equipment used by Quality Pro Test-Consult Ltd. or quoted from relevant international standards.

--- END OF REPORT ---



專業化驗有限公司
QUALITY PRO TEST-CONSULT LIMITED

Unit 10, 5/F, Wah Wai Centre, 38-40 Au Pui Wan St., Fotan, Hong Kong
Email: info@qualityprotest.com; Website: www.qualityprotest.com
Tel: (852) 3956 8717; Fax: (852) 3956 3928

REPORT OF EQUIPMENT PERFORMANCE CHECK/ CALIBRATION

Test Report No. : R-BD010030
Date of Issue : 25 January 2024
Page No. : 1 of 2

PART A - CUSTOMER INFORMATION

Acuity Sustainability Consulting Limited
Unit E, 12/F, Ford Glory Plaza 37-39 Wing Hong Street, Cheung Sha Wan, Kowloon, Hong Kong

PART B - SAMPLE INFORMATION

Name of Equipment : YSI ProDSS (Multi-Parameters)
Manufacturer : YSI (a xylem brand)
Serial Number : 22C106561
Date of Received : 22 January 2024
Date of Calibration : 24 January 2024
Date of Next Calibration : 24 April 2024
Request No. : D-BD010030

PART C - REFERENCE METHODS/ DOCUMENTS FOR THE CALIBRATION

| Test Parameter | Reference Method |
|------------------|---|
| pH value | APHA 21e 4500-H ⁺ B |
| Temperature | Section 6 of international Accreditation New Zealand Technical Guide no. 3 Second edition March 2008: Working Thermometer Calibration Procedure |
| Salinity | APHA 21e 2520 B |
| Dissolved oxygen | APHA 23e 4500-O G (Membrane Electrode Method) |
| Turbidity | APHA 21e 2130 B (Nephelometric Method) |

PART D - CALIBRATION RESULT

(1) pH value

| Target (pH unit) | Display Reading (pH unit) | Tolerance | Result |
|--------------------|-----------------------------|-----------|--------------|
| 4.00 | 4.02 | 0.02 | Satisfactory |
| 7.42 | 7.45 | 0.03 | Satisfactory |
| 10.01 | 10.05 | 0.04 | Satisfactory |

Tolerance of pH value should be less than ± 0.2 (pH unit)

(2) Temperature

| Reading of Ref. thermometer (°C) | Display Reading (°C) | Tolerance | Result |
|------------------------------------|------------------------|-----------|--------------|
| 33 | 34.1 | 1.1 | Satisfactory |
| 19 | 18.7 | -0.3 | Satisfactory |
| 11 | 11.5 | 0.5 | Satisfactory |

Tolerance of Temperature should be less than ± 2.0 (°C)

(3) Salinity


| Expected Reading (g/L) | Display Reading (g/L) | Tolerance (%) | Result |
|--------------------------|-------------------------|-----------------|--------------|
| 10 | 10.19 | 1.90 | Satisfactory |
| 20 | 21.27 | 6.35 | Satisfactory |
| 30 | 30.21 | 0.70 | Satisfactory |

Tolerance of Salinity should be less than ± 10.0 (%)

--- CONTINUED ON NEXT PAGE ---

AUTHORIZED
SIGNATORY:


LEE Chun-ning
Assistant Manager



REPORT OF EQUIPMENT PERFORMANCE CHECK/ CALIBRATION

Test Report No. : R-BD010030
Date of Issue : 25 January 2024
Page No. : 2 of 2

(4) Dissolved oxygen

| Expected Reading (mg/L) | Display Reading (mg/L) | Tolerance | Result |
|---------------------------|--------------------------|-----------|--------------|
| 8.60 | 8.89 | 0.29 | Satisfactory |
| 5.33 | 5.70 | 0.37 | Satisfactory |
| 3.40 | 3.50 | 0.10 | Satisfactory |
| 0.34 | 0.26 | -0.08 | Satisfactory |

Tolerance of Dissolved oxygen should be less than ± 0.5 (mg/L)

(5) Turbidity

| Expected Reading (NTU) | Display Reading (NTU) | Tolerance (%) | Result |
|--------------------------|-------------------------|-----------------|--------------|
| 0 | 0.50 | -- | Satisfactory |
| 10 | 9.88 | -1.2 | Satisfactory |
| 20 | 18.35 | -8.2 | Satisfactory |
| 100 | 95.10 | -4.9 | Satisfactory |
| 800 | 736.55 | -7.9 | Satisfactory |

Tolerance of Turbidity should be less than ± 10.0 (%)

Remark(s)

- The "Date of Next Calibration" is recommended according to best practice principals as practiced by QPT or quoted form relevant international standards.
- The results relate only to the calibrated equipment as received
- The performance of the equipment stated in this report is checked with independent reference material and results compared against a calibrated secondary source.
- "Displayed Reading" denotes the figure shown on item under calibration/ checking regardless of equipment precision or significant figures.
- The "Tolerance Limit" mentioned is the acceptance criteria applicable for similar equipment used by Quality Pro Test-Consult Ltd. or quoted form relevant international standards.

--- END OF REPORT ---